Short Single-Lead ECG Signal Delineation-Based Deep Learning Implementation in Automatic Atrial Fibrillation Identification

by Radiyati Umi Partan

Submission date: 22-Mar-2022 04:40PM (UTC+0700)

Submission ID: 1789999457

File name: plementation in Automatic Atrial Fibrillation Identification.pdf (32.87M)

Word count: 7630

Character count: 41302





Article

Short Single-Lead ECG Signal Delineation-Based Deep Learning: Implementation in Automatic Atrial Fibrillation Identification

Bambang Tutuko ¹, Muhammad Naufal Rachmatullah ¹, Annisa Darmawahyuni ¹, Siti Nurmaini ^{1,*}, Alexander Edo Tondas ², Rossi Passarella ¹, Radiyati Umi Partan ³, Ahmad Rifai ¹, Ade Iriani Sapitri ¹ and Firdaus Firdaus ¹

- Intelligent System Research Group, Faculty of Computer Science, Universitas Sriwijaya, Palembang 30139, Indonesia; bambangtutuko60@gmail.com (B.T.); naufalrachmatullah@gmail.com (M.N.R.); riset.annisadarmawahyuni@gmail.com (A.D.); passarella.rossi@unsri.ac.id (R.P.); ahmadrifai@ilkom.unsri.ac.id (A.R.); adeirianisapitri13@gmail.com (A.I.S.); virdauz@gmail.com (F.F.)
- Department of Cardiology & Vascular Medicine, Dr. Mohammad Hoesin Hospital, Palembang 30126, Indonesia; tondas2000@gmail.com
- Faculty of Medicine, Universitas Sriwijaya, Palembang 30139, Indonesia; radiyati.u.p@fk.unsri.ac.id
- * Correspondence: siti_nurmaini@unsri.ac.id; Tel.: +62-852-6804-8092

Abstract: Physicians manually interpret an electrocardiogram (ECG) signal morphology in routine clinical practice. This activity is a monotonous and 10 tract task that relies on the experience of understanding ECG waveform meaning, including P-wave, QRS-complex, and T-wave. Such a manual process depends on signal quality and the number of leads. ECG signal classification based on deep learning (DL) has produced an automatic interpretation; however, the proposed method is used for specific abnormality conditions. When the ECG signal morphology change to other abnormalities, it cannot proceed automatically. To generalize the automatic interpretation, we aim to delinea 10 CG waveform. However, the output of delineation process only ECG waveform duration classes for P-wave, QRS-complex, and T-wave. It should be combined with a medical knowledge rule to produce the abnormality interpretation. The proposed model is applied for atrial fibrillation (AF) identification. This study meets the AF criteria with RR irregularities and the absence of P-waves in essential oscillations for even more accurate identification. The QT database by Physionet is utilized for developing the delineation model, and it validates with The Lobachevsky University Database. The results show that our delineation model works properly, with 98.91% sensitivity, 99.01% precision, 99.79% specificity, 99.79% accuracy, and a 98.96% F1 score. We use about 4058 normal sinus rhythm records and 1804 AF records from the experiment to identify 49 conditions that are taken from three datasets. The comprehensive testing has produced higher negative predictive value and positive predictive value. This means that the proposed model can identify AF conditions from ECG signal delineation. Our approach can considerably contribute to AF diagnosis with these results.

Keywords: delineation; electrocardiogram; convolutional neural network; long-short term memory



Citation: Tutuko, B.; Rachmatullah, M.N.; Darmawahyuni, A.; Nurmaini, S.; Tondas, A.E.; Passarella, R.; Partan, R.U.; Rifai, A.; Sapitri, A.I.; Firdaus, F. Short Single-Lead ECG Signal Delineation-Based Deep Learning: Implementation in Automatic Atrial Fibrillation Identification. Sensors

10.3390/s22062329 Academic Editors: Mukesh Prasad, Jian Cao, Chintan Bhatt, Monowar

H. Bhuyan and Behnaz Ghoraani

Received: 28 January 2022

Accepted: 14 March 2022

Published: 17 March 2022

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (https://creativecommons.org/licenses/by/4.0/).

1. Introduction

Electrocardiogram (ECG) is the gold standard for signal detection and an effective way to evaluate the heart's rhythm due to its versatility and affordability as a rapid and straightforward test, even in places with scarce resources [1–3]. The test results obtained from an ECG device are heart rhythms, which can reveal an overview of the heart's morphology, such as its structural and physiological conditions [3,4]. A short single-lead ECG is used for essential heart rhythms monitoring, which has a short or minimum duration (seconds) in ECG recording. Additionally, it presents only in one lead ECG signal. It is different to a standard long 12-lead ECG, which provides a complete picture of

Sensors 2022, 22, 2329 2 of 16

heart activity for making clinical decisions [2]. Long ECG tends to need several rounds of recording (minutes to hours) to monitor the morphology. However, health care systems emphasize simple, cost-effective solutions, scalable with automated analysis [5,6]. Several simple, low-cost, wireless wearable ECG mobile devices with a still single-lead analysis have made private screening indispensable [5]. Unfortunately, it is difficult to perform rapid and accurate diagnosis by using such devices, caused by inconsistent findings or low-wave amplitude. About 27% uninterpretable intervals due to single-lead ECG have low quality, noise, low amplitude, complexity, and non-linear characteristics [5,7]. Hence, deep investigation into ECG signal processing is needed to improve the prediction with a short single-lead devicate

The morphology of a normal ECG signal indicates a P-wave, the QRS complex, and a T-wave in the interval of one heartbeat [4]. A normal ECG signal without irregular fluctuations signified a healthy patient. This is different to several heart abnormalities while can be detected by recognizing and analyzing these irregularity characteristics, such as long QT syndrome, which is characterized by a QT interval [5], and atrial fibrillation (AF) with missing P-wave [6]. The human interpretation about AF condition ECG recordings varies widely, although the acquisition has been standardized. This is due to differences in the interpreter's experience and expertise. In addition, human errors and inaccurate interpretations can occur [7,8]. General clinicians missed 20% of AF cases (20 of 99) on a 12-lead ECG and misinterpreted normal sinus rhythm (NSR) as AF by 8% (114 of 1355) when compared to the cardiologist reference standard [9]. The use of single-lead ECGs can increase sensitivity with interpretive software approaches and general clinicians' interpretatio [13] 10]. While ECG signals and patterns are mainly unrecognizable by human interpreters, artificial intelligence (AI) plays a role in precision, making the ECG a robust non-invasive biomarker [11].

In the future, the amount of data generated by the ECG device to be analyzed and diagnosed will increase with the development of sensitivity sensors and other supporting devices, such as cell phones, smartwatches, and low-cost mobile ECG devices [12,13]. Therefore, using AI technology in short single-lead ECG devices will improve quality detection and reduce the burden of analyzing cardiac data. AF condition can be diagnosed using an ECG device that is identified through electrical activity during the repolarization and de 22 arization process. In this study, such process is represented by segmenting the duration of ECG signal waveforms (P-wave, QRS complex, T-wave) named delineation [14]. Proper and correct delineation model for ECG waveform can produce accurate diagnostics [8,15].

Currently, the AI approach with deep learning (DL) algorithms, such as deep neural networks (DNNs) [11,12] convolutional neural networks (CNNs) [13], and recurrent neural networks (R7Ns) [15,16], has revolutionized the way machines interpret ECG signals. RNNs with long short-term memory (LSTM) architecture are an excellent method for exploiting the time-series-based sequential data structures of ECG signals. Using an LSTM architecture with a powerful technique in ECG signal delineation classifies the ECG waveform from one step to the next time step for each heartbeat [14]. However, the lack of feature extraction in LSTI 11 hakes the obtained results less optimal. This study proposes a deep structure of a CNNs as a feature extraction and LSTM as a classifier model to overcome this limitation. The convolutional layers automatically ex 10 these ECG features, and LSTM classify the waveforms into four distinct component waveforms (i.e., P-wave, QRS complex, T-wave, and isoelectric line) in each heartbeat.

In most previous studies, the proposed delineation process is only for localizing and classifying the ECG rhythm without interpreting abnormalities. This study proposes a delineation process for identifying the rhythm abnormality of AF. To our knowledge, no previous study has investigated AF square with a delineation approach. The important finding in our research is that we used a single model architecture to simultaneously predict the presence or absence of all labels and interpret the entire ECG waveform. The final post-processing step is reconciling and aggregating the information from the ECG waveform.

Sensors 2022, 22, 2329 3 of 16

forms and groviding a comprehensive analysis of the signal to make an AF interpretation. Therefore, this study and the proposed method make the following new contributions:

- To propose a framework of automatic identification with a single-lead ECG-based delineation approach.
- To develop the stacked CNNs-Bi-LSTM architecture for ECG waveform delineation with a massive amount of data.
- To implement the combination of delineation approach and medical knc 50 edge base learning to aggregate the information in an ECG signal simultaneously to detect the absence of P-wave, the ventricular response, and the irregularity of the RR interval.
- To evaluate the proposed model for automatic AF interpretation with clinical data pm single-lead personal ECG devices.

With a detailed approach to the problem and to describe the proposed method and its contribution, this paper is structured as follows: In Section 2, we present materials and methods proposed for ECG delineation in identifying AF, while in Section 3, we present the results of applying the methods and a discussion. Finally, Section 4 draws conclusions from the process and the obtained results.

2. Methodology

This section describes our proposed methodology for AF identification, utilizing a delineation process. A sophisticated conceptual framework is proposed by incorporating various established processes to facilitate the ECG waveform delineation and identification of AF. Two blocks are represented in the framework: (i) ECG waveform signal delineation process and (ii) AF screening by interpreting ECG delineation result and medical knowledge representation. The ECG delineation and AF identification process pipeline consists of various stages, as shown in Figure 1. At the delineation base the, we used an ECG signal in normal sinus rhythm (NSR) to classify four waveforms, i.e., P-wave, QRS complex, T-wave, and isoelectric line (no wave). The isoelectric line is the baseline of the ECG, recorded in the TP interval during rhythm with P-waves. The whole methodology is described in the next sub-section as follows.

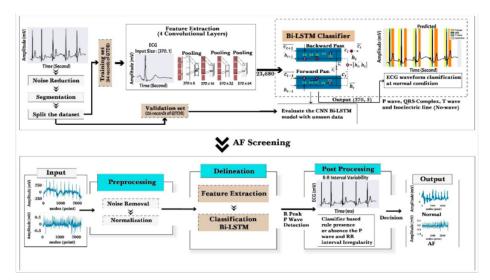


Figure 1. The proposed framework with ECG the delineation approach and AF identification. Automated ECG signal delineation is developed with convolutional layers as feature extraction and Bi-LSTM as a classifier.

Sensors 2022, 22, 2329 4 of 16

2.1. Dataset Preparation

The proposed delineation method was validated on two well-known annotated databases QT Database (QTDB) [17] and a lead II ECG from The Lobachevsky University Database (LUDB) [18]. In comparison, AF identification utilized the PhysioNet/CinC Challenge 2017 database [19], The China Physiological Signal Challenge 2018 database [20], and ECG recordings from Mohammad Hoesin Indonesia General Hospital. The whole data distribution is seen in Table 1.

Table 1. The data distribution for	the delineation and	identification process.
---	---------------------	-------------------------

Database	Records	Description	Frequency Sampling
	Delineation Mo	del	
QTDB	10 subjects NSR 15 subjects Arrhythmias Two subjects NSR	Training/validation Training/validation Testing	250-500 Hz
LUDB	200 subjects for NSR, tachycardia, bradycardia, arrhythmia, irregular rhythm, AF, atrial flutter	Other data set for model validated	500 Hz
	Medical knowledge-bas	ed learning	
PhysioNet/CinC Challenge 2017 database	5154 subjects NSR	AF identification	300 Hz
	771 subjects AF		
The China Physiological Signal Challenge 2018 database	918 subjects NSR 1098 subjects AF	AF identification	500 Hz
ECG recordings from Mohammad Hoesin Indonesian Hospital.	78 subjects NSR	AF identification	300 Hz

2.2. Noise Removal

29 dor pois

The baseline wander noise must be removed from the raw signal to produce satisfactory results from the delineation process. 35 see factors were removed by applying a discrete wavelet trans 36 mation (DWT) with low-pass and high-pass filters [14,21]. This strategy can separate the ECG signal into various frequency bands and maintain a good representation of a nonstationary signal [7,22]. While each signal is decomposed per level to remove ECG noise, DWT produces half of the input signal frequency. This process was conducted in approximately eight stages of decomposition. The noise removal process was carried out using soft-thresholding techniques and universal-threshold rules for each signal decomposition. The decomposition results were reconstructed back into the initial signal cleaned of noise.

2.3. Segmentation

Segmentation is a crucial stage in the delineation process for classifying the whole waveform pattern of the ECG signal. The process is conducted by dividing the short single-lead ECG signal into a beat-to-beat segment to achieve a proper window size. Segmentation started from the P-wave and went to the isoelectric line after the T-wave, which contained one heartbeat at an NSR heart rate. These segment points were sampled with around 250 Hz for three beats. However, it should be noted that the continuity of the time series (ECG signal) within each segment was preserved to make it workable for the network to learn the pattern of different waveforms from each input. After the beat-by-beat segmentation process, we have the data for the delineation process, as seen in Table 2.

Sensors 2022, 22, 2329 5 of 16

Table 2. The ECG beat segmentation to develop the delineation model.

Data	Training (Beats)	Validation (Beats)	Testing (Beats)
QTDB	14,376	1639	100
LUDB	1096	122	-

2.4. CNN-Bi-LSTM

A previous study achieved best performance when the ECG signal was delineated automatically with a CNNs and bidirectional LSTM (Bi-LSTM) architecture [21]. A unidirectional phase also has limits because future input information is impossible to get from the current state. On the other hand, bidirectional does not necessitate correcting its input data. Furthermore, the current state allows access to future input data [23]. The feature extraction of CNNs process used four convolutional layers without max pooling. The convolution process can be expressed as follows [7,21]:

$$a_{ij}^{m} = \varphi(b_i + \sum_{k=1}^{M} w_{ik} x_{j+k-1}) = \varphi(b_i + w_i^T x_j)$$
 (1)

where a_{ij}^m is the activation of the j neuron of the i filter for the m convolutional layer, Mis the kernel size [8], φ is the neural activation function, b is the shared bias of the i filter, $w_i = \begin{bmatrix} w_{i1} & w_{i2} & \dots & w_{iM} \end{bmatrix}^T$ are the shared weights of the *i* filter, and $x_j = \begin{bmatrix} x_j & x_{j+1} & \dots & x_{j+M-1} \end{bmatrix}^T$ are the corresponding *M* inputs.

In this study, the convolutional layer received two input values: the ECG beats and corresponding labels, including P-wave, QRS complex, T-wave, isoelectric line (no wave), and zero padding. The ECG beat had a size of (370, 1), which contains information about the class type of each ECG node. We divided the classes into P-wave as class 0, QRS complex as class 1, T-wave as class 2, the isc 43 ctric line (no wave) as class 3, and zero padding as class 4. The network was combined with the rectified linear unit (ReLU) activation function. This function has been adopted with four convolution layers (8, 16, 32, and 64 filters), resulting in an output size (370, 64). This output size means that the features were set into 370 timesteps, containing 64 features per timestep. The output from the convolutional part was adjusted to feed into the Bi-LSTM part as a classifier. We used the OneHotEncoder() function to encode categorical features as a one-hot numeric array, resulting in a shape of (370, 5). The one-hot array was then fed into the Bi-LSTM classifier model as a target along with the ECG waveform as an input. The feature map resulting from the convolutional layers is shown in Figure 2.

The p3 posed model is to classify the positions and magnitudes of the following durations, such as P-wave, QRS complex, and T-wave. The Bi-LSTM architecture processes a data sequence in both directions by two hidden layers, which are fed forward to the output layer and backward along with their corresponding weights (W) and biases (b). Two parallel directions of forwarding and backward passes are provided below [21].

$$a^{t} = \tanh(W_c x^t + U_c h^{t-1}) \tag{2}$$

$$i^{t} = \sigma(W_{i}x^{t} + U_{i}h^{t-1}) = \sigma(\hat{i}^{t})$$
(3)

$$f^{t} = \sigma(W_{f}x^{t} + U_{f}h^{t-1}) = \sigma(\widehat{f}^{t})$$

$$\tag{4}$$

$$o^{t} = \sigma(W_{o}x^{t} + U_{o}h^{t-1}) = \sigma(\widehat{o}^{t})$$
(5)

$$o^{t} = \sigma(W_{o}x^{t} + U_{o}h^{t-1}) = \sigma(\widehat{o}^{t})$$

$$LSTM_{ft}^{\rightarrow 1} = \tanh(W_{ih}^{1}x_{t} + W_{hh}^{1}LSTM_{t-1}^{1} + b_{h}^{1})$$

$$(5)$$

$$LSTM_{bt}^{\leftarrow 1} = \tanh(W_{ih}^{1} x_{t} + W_{hh}^{1} LSTM_{t+1}^{\leftarrow 1} + b_{h}^{\leftarrow 1})$$

$$(7)$$

Sensors 2022, 22, 2329 6 of 16

From Equations (6) and (7), the output of the Bi-LSTM layer at a time *t*:

$$y_{t}^{1} = \tanh(W_{ho}^{1} LST \overrightarrow{M}_{t}^{1} + W_{ho}^{1} LST \overrightarrow{M}_{t}^{1} + b_{0}^{1})$$
 (8)

where a^t is input, i^t is input gate, f^t is forget gate, o^t is output gate, h is hidden gate, the output depends on $LSTM_t$ and $LSTM_t$; h_0 is initialized as a zero vector.

In the process of ECG waveform classification, a fixed window size of 370 node 20 pr each sequence was used. The window size was large enough to capture one heartbeat (from the 25rt of P-wave 1 to the start of P-wave 2). The total of the nodes' starts-to-end index of the P-wave, QRS complex, T-wave, and the isoelectric line hall to be adjusted in the unit of seconds, respectively. These duration points were sampled with a sampling frequency of about 250 Hz. The classifier architecture used in this study consisted of an input layer size (370, 1) with five output layers, producing 512 hidden layer neurons, including the Tanh-Sigmoid hidden activation function. The output layer activation function was Softmax, with a learning rate of 0.0001 and the epoch was 300. The network optimizer utilized was the Adam optimizer, and categorical cross-entropy was selected as a loss function to measure the loss value of the classifi 48 nodel. The output from this classifier contains the probability class for each node. One class with the highest probability value was selected as the predicted output of the model. In the end, a vector with a size of (370, 1) was formed as the predicted class of each node.

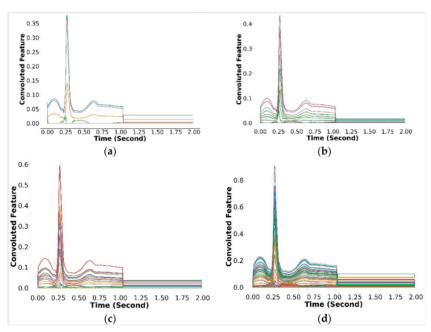


Figure 2. The result of the feature map from convolutional layers. (a) Convolution 1 (370, 8). (b) Convolution 2 (370, 16). (c) Convolution 3 (370, 32). (d) Convolution 4 (370, 64).

The entire structur 47 the feature extraction and classification process by the CNNs-Bi-LSTM architecture is shown in Table 3.

Sensors 2022, 22, 2329 7 of 16

9 Layer	Input Nodes	Filter Number	Kernel Size/Pool Size	Output Nodes	Feature Interpretation
Input	370, 1	-	-	-	ECG amplitude for one beat
Convolution 1	370×1	8	3×1 , stride 1	370 × 8	8 feature maps
Convolution 2	370 × 8	16	3×1 , stride 1	370 × 16	16 feature maps
Convolution 3	370 × 16	32	3×1 , stride 1	370 × 32	32 feature maps
Convolution 4	370 × 32	64	3×1 , stride 1	370×64	64 feature maps
Bi-LSTM	370 × 64	-	-	370 × 1024	Two directions of feature data (512 nodes for both forward and backward directions)
Output	-	-		370 × 5	370 nodes with five classes (P-wave QRS-complex, T-wave, No-wave, and zero padding)

Table 3. The structure of the proposed CNNs-Bi-LSTM architecture.

2.5. Model Delineation E-pluation

The performance of the proposed Bi-LSTM model was validated using a confusion matrix. To evaluate classification performance, we applied performance metrics [24,25]. Furthermore, we used a positive predictive value (precision) versus a sensitivity (recall) or precisio 33 recall (P–R) curve to measure all potential cut-offs in the delineation process. The higher area under the curve (AUC) value was the 33-R curve [24]. For model configuration and evaluation, we conducted the experiments on a wo 40 tation with one Intel(R) Core (TM) i7-10700K CPU, with a 3.80 GHz processor and 32 GB RAM, and one NVIDIA GeForce RTX 2070 Super 8 GB GPU. All experiments were run on Windows 10 Pro 64-Bit and CuDNNLSTM.

2.6. AF Identification

In measuring the diagnostic performance of AF, it is common to leverage an ECG, a signal that measures the heart's electrical active As shown in Figure 3, a special hallmark of AF in the absence of P waves is that the rhythm is irregularly irregular, and the morphology of the P-waves is fibrillation [24]. This study conducted two important stages for making an automatic AF interpretation from the ECG signal: detecting the heart-rate variability (HRV) to measure the regular or irregular condition and detecting the presence or absence of P-waves in the ECG record to support AF interpretation.

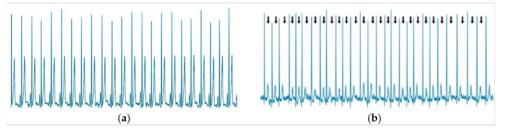


Figure 3. Example of ECG signal: (a) normal rhythm as NSR and (b) abnormal rhythm as AF.

An AF identification procedure after ECG signal delineation is as follows:

- Each ECG device has a different frequency sampling and to produce the generalization model of delineation, to determine one beat, it was segmented again around 0.2 s before the R_{peak} and 0.45 s after the R_{peak}.
- From the delineation result, we can determine the occurrence P-wave pattern; however, the QRS complex should be processed to determine heart-rate irregularity. To

Sensors 2022, 22, 2329 8 of 16

measure the distance between R_{peak} - R_{peak} or RR, intervals were calculated using the following equation:

$$RR^{Interval} = (R_{peak}[i] - R_{peak}[i+1]) * fs * 1000$$
 (9)

where $R_{peak}[i]$ is R_{peak} position at i node, $R_{peak}[i+1]$ is R_{peak} position at (i+1) in nodes, fs is the frequency sampling, and RR interval values in beat per minutes (BPM).

- From the RR interval result, the ECG signal was checked to determine whether there
 was a continuous change in ventricular response in five to seven beats to indicate
 whether the ECG has a regular or an irregular rhythm in the ECG recording.
- The three BPM ranges of ventricular response are needed to ensure whether a signal is normal or AF condition, as (i) the normal ventricular response group has the RR interval value ranged between 60 and 100 BPM; (ii) the slow ventricular response group has the RR interval value less than 60 BPM (<60 BPM); and (iii) the rapid ventricular response group has the RR interval greater than 100 BPM (>100 BPM).
- After determining the ventricular response of the ECG signal, then the regular or irregular rhythm is determined. An ECG signal is said to be a Regular Rhythm if that rhythm has a pattern. The rhythm pattern can be a normal, rapid, or slow ventricular response. On the other hand, if there is no pattern occurred in the ECG signal, then the signal is categorized as an irregular rhythm.
- By using two inputs, the AF or NSR was interpreted according to the following rules:
 - If the P-wave was present and the rhythm regular, then the condition was normal.
 - If the P-wave was absent and the rhythm regular, then the condition was normal.
 - If the P-wave was present and the rhythm irregular, the condition was AF.
 - If the P-wave was absent and the rhythm irregular, the condition was AF.

3. Results and Discussion

25 orphology in the ECG signal can be represented by the cardiac waveform series of the P-wave, the QRS complex, the T-wave, and the isoelectric line (no wave). This study has proposed a training, validation, and testing set for the delineation task. The validation set is used for the hyperparameter tuning, while the testing set as unseen data is used to show the generalization abilities of the CNNs-Bi-LSTM model.

This study classified such a waveform series using 90% for the training process and 10% for the testing process with shuffle sampling. The total training set was 7714 samples, and the testing set was 858 samples. The CNNs-Bi-LSTM result was compared to the data annotation by *ecgpuwave* in the QTDB, and we also compared the LSTM and Bi-LSTM classifiers without feature extraction. The *ecgpuwave* provided the exact location of all waveforms in the signal. The *ecgpuwave* output was written as a standard WFDB-format annotation file related to the specified annotator that was utilized as label or 'ground truth' for ECG waveforms.

3.1. Model Evaluation of the Delineation Process

The LSTM standard has a unidirectional phase that preserves the past information and runs the inputs only in forward passes. In contrast, the Bi-LSTM phase runs inputs in forward and backward passes and preserves the information from both the past and future. Figures 4 and 5 show the performance of the proposed CNNs-Bi-LSTM classifier in the training and validation evaluation. All classification performances reached over 99% in the training phase. Only the T-wave classification produced 98.75% precision, 98.12% sensitivity, and a 98.44% F1-score in the validation phase, while the remaining achieved over 99%.

Sensors 2022, 22, 2329 9 of 16



Figure 4. Model evaluation for the training process in normal ECG waveform.

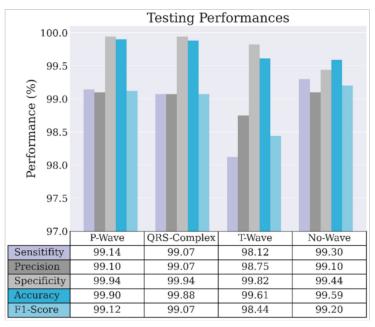


Figure 5. Model evaluation for the validation process in normal ECG waveform.

Three scenarios were created to validate the pro_4 sed model with an intra-inter patient in normal rhythm and arrhythmia conditions. Most previously reported works on medical data in the literature have been evaluated only for the intra-patient paradigm rather than the inter-patient scheme, which is a more realistic scenario to prevent training and to test the model using samples from the same patients. Therefore, some of these

Sensors 2022, 22, 2329 10 of 16

methods achieved good accuracy using the intra-patient scheme; however, their results are unreliable, as their evaluation process was biased. In addition, the input data has never been recognized in the training process in the testing processes that use inter-patient data. In some cases, it can cause the performance results to decrease significantly.

The waveform classification performance of the three scenarios is shown in Table 4. By using inter-patient data, the CNNs-Bi-LSTM model has maintained classification performance. However, in the inter-patient (NSR) scenario, the sensitivity decreased by about 9%, and the precision decreased by about 4%. Such conditions happened due to the interpatient data having variations in signal morphology, and the noise suppressed the ECG 20 al. We also tested the delineate system with abnormal data in the arrhythmia condition 14 ntricular premature complexes and atrial premature complexes). Ventricular and atrial premature complexes occur when the lower chambers of the heart contract before they should. When this happens, the heartbeat becomes out of sync. This can produce a regular heartbeat, an extra heartbeat, a pause, and a stronger heartbeat. With such an arrhythmia condition, our model delineation performance decreased 1.47% in sensitivity, 1.48% in precision, 0.28% in specificity, and 0.48% in accuracy (see Table 4). However, our model still maintained performance over 97% in sensitivity, which means that the model produces a high true positive rate value.

Table 4. Delineation results in an intra–inter patient with NSR, arrhythmia, and various conditions using the QTDB and the LUDB.

Database	Records	Scenario -		Classific	cation Perform	ance (%)	
Database	Records	Scenario -	Sen.	Prec.	Spec.	Acc.	F1-Score
	10	Intra-patient (NSR)	98.91	99.01	99.79	99.79	98.96
QTDB	15	Intra-patient (Arrythmia)	97.44	97.53	99.57	99.31	97.48
	2	Inter-patient (NSR)	89.90	94.30	97.86	97.33	91.70
LUDB	200	Intra-patient (Various Conditions)	95.61	95.93	99.18	98.77	95.76

Note: Sensitivity (Sen.), Precision (Prec.), Specificity (Spec.), Accuracy (Acc.).

For another experiment with the same hyperarameters, the ECG signals of the LUDB were implemented in an intra-patient scenario to analyze the performance comparison of the delineation are conditions, such as situs rhythm. All the LUDB recordings were validated under various conditions, such as situs rhythm, sinus tachycardia, sinus bradycardia, sinus arrhythm, irregular sinus rhythm, AF, and atrial flutter. With the massive data of the LUDB, the performance of the delineation algorithm was applied in various conditions, and all performances were achieved above 95.61%. Thus, the proposed CNNs-Bi-LSTM model was still robust for the delineation task, and there was no significant gap between the QTDB and the LUDB in the intra-patient scenario (see Table 4). The performance dectage witnessed by using the LUDB could be due to various signal abnormalities, such as Sinus Rhythm, Sinus Tachycardia, Sinus Bradycardia, Sinus Arrhythmia, Irregular Sinus Rhythm, AF, and Atrial Flutter. The enormous difference in recorded numbers could be more challenging. The LUDB had 200 records, while the QTDB used only 10 and 15 records for NSR and arrhythmia, respectively. Hence, the LUDB offers a variety of complex morphologies, which can be a challenge in the delineation process.

For QTDB, the confusion matrices for NSR with inter-patient cases showed that the P-wave class was misclassified in about 315 samples, the QRS complex in about 145 samples, and the T-wave in about 1006 samples (refer to Figure 6a). This meant that the nodes shifted from all samples to the isoelectric line; however, no sample was misclassified into another waveform class. When testing for the arrhythmia condition, as shown in Figure 6b, the QRS complex class was misclassified as another waveform class, three samples were misclassified as P-waves, and 13 samples were misclassified as T-waves. However, due to

Sensors 2022, 22, 2329 11 of 16

the large number of 35 G recordings in the MIT-BIH Arrhythmia dataset, the waveform classification results in terms of their sensitivity and precision performances still reached over 97% (see Tast 4). The shift of the waveform class to the isoelectric line class occurred in three classes: P-wave 10 RS complex, and T-wave. On the other hand, when the model was validated in LUDB, P-wave, QRS-complex, and T-wave were misclassified as isoelectric lines (refer to Figure 6c).

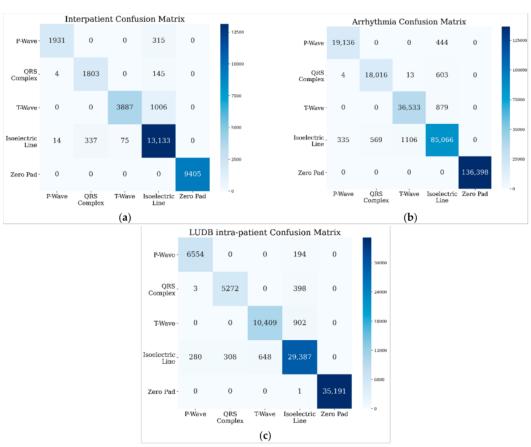


Figure 6. Confusion matrices for QTDB's (a) inter-patient and (b) arrhythmia conditions, and (c) LUDB's intra-patient.

Figure 7a,b shows another metric of delineation performance in the intra- and interpatient scenarios: the precision–recall (P–R) curve to evaluate experimental performance. Precision can be seen as quality, whereas recall can be seen as a measure of quantity. The P-R curve was essential in this study because the ECG delineation had four classes of waveforms and zero padding along with the signal. Therefore, the shift in each class duration will affect the delineation process's precision performance.

The P-R curve was utilized to show the false positive and false negative rate values. The two curves show good results utilizing CNNs-Bi-LSTM models. The intra-patient data produces an average P-R curve area of 1.0 a 15 the inter-patient data, producing an area of 0.98, which shifts to the upper right. The high area under the curve (AUC) represents both high recall and precision, where high precision relates to a low false-positive rate and high recall relates to a low false-negative rate. In the intra-patient data 33 classes produced an AUC of over 97%. However, in the inter-patient data, the AUC of the QRS

Sensors 2022, 22, 2329 12 of 16

complex and T-wave reached 85% and 80%, respectively. This means that the duration of the two waves shifted by 13–17% to the isoelectric line or no-wave class. There were no positive or negative electrical charges to create deflections.

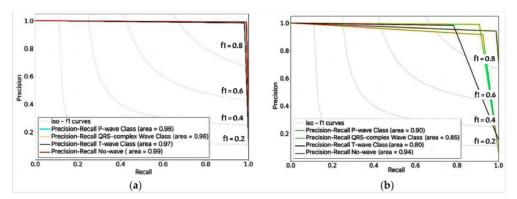


Figure 7. Model evaluation based on precision–recall (P–R) curves. **(a)** intra-patient data. **(b)** inter-patient data.

Figure 8 depicts a sample delineation result of one beat in the NSR with intra–interpatient data for QTDB. The result appeared to indicate a satisfactory waveform pattern; however, in the long ECG signal recording, the wave's duration shifted to the isoelectric line in a large amount of inter-patient data. This must be improved significantly to produce exact waveform delineation results (see Table 4).

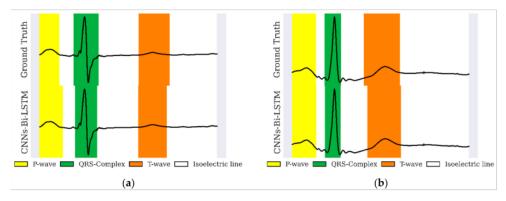


Figure 8. A sample of one-beat ECG signal delineation results for (a) intra-patient and (b) interpatient in NSR data. Each figure represents the QTDB ground truth (top figure) and CNNs-Bi-LSTM (bottom figure).

This work presents a CNNs-Bi-LSTM-based approach for ECG delineation by framing the problem as a classification task. Our work exhibits good delineation performance, and the network has excellent classification performance in single-lead scenarios with unseen data (inter-patient), as depicted in Figure 9. Our approach is data-driven. Therefore, any bias in the QTDB will be learned by the network. In this sense, CNNs-Bi-LSTM-based approaches, such as the proposed model, can easily assimilate newly annotated data to enhance delineation performance. Development became shortened once the right design decisions had been modeled, thus becoming an alternative to DL-based methods with great potential. In Figure 9, we plotted the sample of delineation results in four beats. The classification results showed satisfactory performance. CNNs-Bi-LSTM can recognize

Sensors 2022, 22, 2329 13 of 16

several ECG morphologies in terms of P-wave, QRS complex, and T-wave, along with a signal recording.

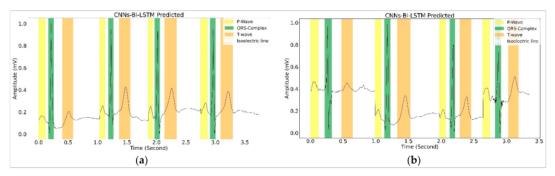


Figure 9. The four-beat sample of ECG-signal delineation in (a) NSR and (b) arrhythmia.

We compared the proposed delineation process with two other networks: unidirectional (Uni-LSTM) and Bi-LSTM architectures without CNNs. The feature extraction performed by convolutional layers can improve the proposed model's classification performance (see Table 5). The average precision classification of the waveform increased from 98.97% to 99.01% using the proposed model, and the other metrics also increased. In addition, we compared our proposed model to other delineation task (see Table 6). Based on the results for the P-wave, QRS complex, and T-wave detection, the performance in our delineation model significantly outperformed the other methods proposed by [14,25] and [15] due to all their methods reaching metrics under 98%.

Table 5. The three LSTM architectures with the best result.

Architecture		Po	erformance (%)	
Architecture	Sen.	Prec.	Spec.	Acc.	F1-Score
Uni-LSTM	98.71	98.80	99.75	99.64	98.75
Bi-LSTM	98.84	98.97	99.68	99.68	98.91
Convolutional-Bi-LSTM	98.91	99.01	99.79	99.79	98.96

Note: Sensitivity (Sen.), Precision (Prec.), Specificity (Spec.), Accuracy (Acc.).

Furthermore, while the performance results obtained by [26,27] were excellent (around 99%), their detection focused only on the QRS complex. Our study generated the delineation algorithm for the P-wave, QRS complex, T-wave, and isoelectric line (no wave). 27 ethree main deflections of ECG waveforms are essential for practical diagnosis. The P-wave is caused by the depolarization wave spreading over both a 13. The QRS complex is written when the depolarization wave reaches the ventricles. A period of electrical inactivity follows, during which the ECG records the ST segment. Finally, the ventricular muscle slowly recharges in preparation for the extraction of the ventricles appears as a T-wave. Thus, it can be concluded that our proposed model had a good result in the delineation process in the inter-patient data of the QTDB, with all performances achieving above 98.91% (see Table 6).

Sensors 2022, 22, 2329 14 of 16

Table 6. Comparison with other delineation using deep learning model with the same QTDB records.

Architecture	Detection -		I	Performance (%	b)	
Architecture		Sen.	Prec.	Spec.	Acc.	F1-Score
Convolutional LSTM [7]	P-wave, QRS-complex,	97.95	95.68	-	-	96.78
Convolutional Neural Network-UNet [25]	P-wave, QRS-complex, and T-wave	99.51	95.83	-	-	-
Convolutional Long Short-Term Memory [15]	P-wave, QRS-complex, and T-wave	94.47	94.19	-	94.75	94.66
Convolutional Neural Network [26]	QRS-complex	99.97	99.99	-	-	99.98
Convolutional Neural Network [27]	QRS-complex	99.10	99.00	-	-	-
Proposed model	P-wave, QRS-complex, T-wave, and Isoelectric line (no-wave)	98.91	99.01	99.79	99.79	98.96

Note: Sensitivity (Sen.), Precision (Prec.), Specificity (Spec.), Accuracy (Acc.).

3.2. AF Identification Results

We conducted experiments for AF identification with three datasets taken from (i) the China Physiological Signal Challenge 2018, (ii) the PhysioNet Computing in Cardiology Challenge 2017, and (iii) the Mohammad Hoesin General Hospital Indonesia. The three datasets have different sampling frequencies 42 heir ECG recordings. Meanwhile, the design delineation model uses the NSR QTDB with a sampling frequency of 250 Hz. The difference between the data model and the data tested will be challenging because it will affect the nodes generated in each beat. AF can be identified by confirming three decision-making factors: the P-wave's absence in duration 0.06–0.08 s and considerably higher beats per minute than 60–100 BPM with inconsistent RR interval variations and not within the 0.6–1.0 s range [27]. The identification results were evaluated based on positive predictive value (PPV) or the probability that subjects with a positive screening test truly have the disease. A negative predictive value (NPV) is the probability that subjects with a negative screening test truly do not have the disease. The AF identification results can be summariated as follows:

- The China Physiological Signal Challenge 2018 database was collected from 11 hospitals and contained 12-lead ECG recordings lasting 6–60 s, this study used only lead II. In the identification process, we used about 826 NSR records and 988 AF records. The results showed that we had 95.40% PPV, 84.55% NPV, and an 89.65% F1-score. There were 38 (4.6%) records that had a false negative (FN), and 144 (14.5%) records that had a false positive (FP).
- The PhysioNet Computing in Cardiology Challenge 2017 database was collected from a short single-lead ECG recording between 30 and 60 s in length. ECG recordings were collected using a mobile Cardia with the AliveCor device. We utilized about 3154 NSR records and 771 AF records. The experiment reached 86.51% PPV, 95.95% NPV, and an 90.43% F1-score. There were 457 (14.4%) records with FN and 114 (1.4%) records with FP.
- The Gen 19 Mohammad Hossein Hospital (Palembang, Indonesia) database was collected from a short single-lead ECG recording between 30 and 60 s in length. ECG recordings were collected using a mobile Cardia with the AliveCor device. We utilized about 78 NSR records and 45 AF records. The experiment reached 85.61% PPV, 97.10% NPV, and a 90.41% F1-score. There were 12 (15.3%) records with FN and two (4.4%) records with FP.

Sensors 2022, 22, 2329 15 of 16

A short single-lead ECG dem 23 strated an overall greater NPV or sensitivity value from the experiment. This means that the proposed model makes it possible to identify cardiac abnormalities from a single-lead ECG, even when the recordings are of short duration, with delineation and 3 edical knowledge representation. One of the questions this work has addressed is the clinical impact that this method can achieve. Thus, it was critical to evaluate the model in a real dataset known for its many patients and signals. Even though we are critical of some of the manual annotations in the QTDB from PhysioNet, we assume that most of the annotations are correct and can be used for evaluation. The main limitation of this work is the lack of more up-to-date databases that contain a higher variability for a more comprehensive array of pathologies. Despite ECG usually being the first information registered of a patient's cardiac condition, not many large, annotated databases for ECG delineation exist.

4. Conclusions

This research aimed to develop a non-invasive method to detect AF conditions using a single-lead ECG signal delineation approach. Although we did not test the proposed model with clinical data, the model was validated and tested with massive data from three datasets. Even though this identification system is not a direct replacement as a standard ECG, the utilization of this affordable system will contribute toward reducing strokes, raising heart health awareness, and significantly saving on costs. The AF identification system will allow physicians with less knowledge of how to evaluate ECG signals or other related factors to get a simple identification of potential AF concerns. The proposed CNNs-Bi-LSTM network demonstrated significant precision in identifying AF with a specific algorithm, and it can be improved as 17 eneralized model for other heart diseases. In the future, further research will focus on how to better integrate physicians' experience and expertise into the DL model to improve the performance of the ECG delineation task, and to generalize our approach to cover more cross-disciplinary work.

Author Contributions: B.T.: Formal analysis and writing—original draft; M.N.R.: Softwar 52 alyst, and review and editing; A.D.: Resources, data analyst and writing—review and editing; § I.: Funding acquisition and writing—review and editing; A.E.T.: Medi 54 data verification; R.P.: Data anal 24 R.U.P.: Medical data verification; A.R.: Data analyst; A.I.S.: Software analyst; F.E.: Data analyst. All authors have read and agreed to the published version of the manuscript.

Funding: This research was funded by Universitas Sriwijaya Indonesia under the competitive grant.

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Data Availability Statement: Not applicable.

Acknowledgments: We thank the Intelligent System Research Group (ISysRG), Faculty of Computer Science, Universitas Sriwijaya, Indonesia, for supporting the financial.

Conflicts of Interest: The authors declare no conflict of interest.

References

- Jonas, D.E.; Kahwati, L.C.; Yun, J.D.; Middleton, J.C.; Coker-Schwimmer, M.; Asher, G.N. Screening for atrial fibrillation with electrocardiography: Evidence report and systematic review for the US preventive services task force. JAMA 2018, 320, 485

 [CrossRef] [PubMed]
- Zheng, J.; Zhang, J.; Danioko, S.; Yao, H.; Guo, H.; Rakovski, C. A 12-lead electrocardiogram database for arrhythmia research covering more than 10,000 patients. Sci. Data 2020, 7, 48. [CrossRef] [PubMed]
- Haverkamp, H.T.; Fosse, S.O.; Schuster, P. Accuracy and usability of single-lead ECG from smartphones—A clinical study. Indian Pacing Electrophysiol. J. 2019, 19, 145–149. [CrossRef] [PubMed]
- Hammad, M.; Zhang, S.; Wang, K. A novel two-dimensional ECG feature extraction and classification algorithm based on convolution neural network for human authentication. Future Gener. Comput. Syst. 2019, 101, 180–196. [CrossRef]
- Hajimolahoseini, H.; Redfearn, D.; Krahn, A. A Deep Learning Approach for Diagnosing Long QT Syndrome without Measuring QT Interval. In Canadian Conference on Artificial Intelligence; Springer: Cham, Switzerland, 2019; pp. 440–445.

Sensors 2022, 22, 2329 16 of 16

 Hagiwara, Y.; Fujita, H.; Oh, S.L.; Tan, J.H.; San Tan, R.; Ciaccio, E.J.; Acharya, U.R. Computer-aided diagnosis of atrial fibrillation based on ECG signals: A review. *Inf. Sci.* 2018, 467, 99–114. [CrossRef]

- Peimankar, A.; Puthusserypady, S. DENS-ECG: A deep learning approach for ECG signal delineation. Expert Syst. Appl. 2021, 165, 113911. [CrossRef]
- 8. Cosoli, G.; Spinsante, S.; Scardulla, F.; D'Acquisto, L.; Scalise, L. Wireless ECG and cardiac monitoring systems: State of the art, available commercial devices and useful electronic components. *Measurement* 2021, 177, 109243. [CrossRef]
- Smith, S.W.; Rapin, J.; Li, J.; Fleureau, Y.; Fennell, W.; Walsh, B.M.; Rosier, A.; Fiorina, L.; Gardella, C. A deep neural network for 12-lead electrocardiogram interpretation outperforms a conventional algorithm, and its physician overread, in the diagnosis of atrial fibrillation. IJC Heart Vasc. 2019, 25, 100423. [CrossRef]
- Mant, J.; Fitzmaurice, D.A.; Hobbs, F.R.; Jowett, S.; Murray, E.T.; Holder, R.; Davies, M.; Lip, G.Y. Accuracy of diagnosing atrial fibrillation on electrocardiogram by primary care practitioners and interpretative diagnostic software: Analysis of data from screening for atrial fibrillation in the elderly (SAFE) trial. BMJ 2007, 335, 380. [CrossRef]
- Nurmaini, S.; Umi Partan, R.; Caesarendra, W.; Dewi, T.; Naufal Rahmatullah, M.; Darmawahyuni, A.; Bhayyu, V.; Firdaus, F. An Automated ECG Beat Classification System Using Deep Neural Networks with an Unsupervised Feature Extraction Technique. Appl. Sci. 2019, 9, 2921. [CrossRef]
- Nurmaini, S.; Darmawahyuni, A.; Sakti Mukti, A.N.; Rachmatullah, M.N.; Firdaus, F.; Tutuko, B. Deep Learning-Based Stacked Denoising and Autoencoder for ECG Heartbeat Classification. *Electronics* 2020, 9, 135. [CrossRef]
- 13. Zhu, F.; Ye, F.; Fu, Y.; Liu, Q.; Shen, B. Electrocardiogram generation with a bidirectional LSTM-CNN generative adversarial network. Sci. Rep. 2019, 9, 6734. [CrossRef]
- Nurmaini, S.; Tondas, A.E.; Darmawahyuni, A.; Rachmatullah, M.N.; Effendi, J.; Firdaus, F.; Tutuko, B. Informatics in Medicine Unlocked Electrocardiogram signal classification for automated delineation using bidirectional long short-term memory. Inform. Med. Unlocked 2021, 22, 100507. [CrossRef]
- Malali, A.; Hiriyannaiah, S.; Siddesh, G.M.; Srinivasa, K.G.; Sanjay, N.T. Supervised ECG wave segmentation using convolutional LSTM. ICT Express 2020, 6, 166–169. [CrossRef]
- Ma, F.; Zhang, J.; Chen, W.; Liang, W.; Yang, W. An automatic system for atrial fibrillation by using a CNN-LSTM Model. Discret. Dyn. Nat. Soc. 2020, 2020, 1–9. [CrossRef]
- 17. Laguna, P.; Mark, R.G.; Goldberg, A.; Moody, G.B. A database for evaluation of algorithms for measurement of QT and other waveform intervals in the ECG. In *Computers in Cardiology* 1997; IEEE: Piscataway, NJ, USA, 1997; pp. 673–676.
- Kalyakulina, A.I.; Yusipov, I.I.; Moskalenko, V.A.; Nikolskiy, A.V.; Kosonogov, K.A.; Osipov, G.V.; Zolotykh, N.Y.; Ivanchenko, M.V. Ludb: A new open-access validation tool for electrocardiogram delineation algorithms. *IEEE Access* 2020, 8, 186181–186190. [CrossRef]
- Goldberger, A.L.; Amaral, L.A.; Glass, L.; Hausdorff, J.M.; Ivanov, P.C.; Mark, R.G.; Mietus, J.E.; Moody, G.B.; Peng, C.K.; Stanley, H.E. PhysioBank, PhysioToolkit, and PhysioNet: Components of a new research resource for complex physiologic signals. Circulation 2000, 101, e215–e220. [CrossRef]
- Liu, F.; Liu, C.; Zhao, L.; Zhang, X.; Wu, X.; Xu, X.; Liu, Y.; Ma, C.; Wei, S.; He, Z.; et al. An open access database for evaluating the algorithms of electrocardiogram rhythm and morphology abnormality detection. J. Med. Imaging Health Inform. 2018, 8, 1368–1373.
 [CrossRef]
- Nurmaini, S.; Darmawahyuni, A.; Rachmatullah, M.N.; Effendi, J.; Sapitri, A.I.; Firdaus, F.; Tutuko, B. Beat-to-Beat Electrocardiogram Waveform Classification Based on a Stacked Convolutional and Bidirectional Long Short-Term Memory. *IEEE Access* 2021, 9, 92600–92613. [CrossRef]
- Almumri, A.; Balakrishnan, E.; Narasimman, S. Discrete Wavelet Transform Based Feature Extraction in Electrocardiogram Signals. Glob. J. Pure Appl. Math. 2021, 17, 63–77.
- Darmawahyuni, A.; Nurmaini, S.; Rachmatullah, M.N.; Firdaus, F.; Tutuko, B. Unidirectional-bidirectional recurrent networks for cardiac disorders classification. *Telkomnika* 2021, 19, 902–910. [CrossRef]
- Ghorbani, A.; Ouyang, D.; Abid, A.; He, B.; Chen, J.H.; Harrington, R.A.; Liang, D.H.; Ashley, E.A.; Zou, J.Y. Deep learning interpretation of echocardiograms. NPJ Digit. Med. 2020, 3, 10. [CrossRef] [PubMed]
- Jimenez-Perez, G.; Alcaine, A.; Camara, O. Delineation of the electrocardiogram with a mixed-quality-annotations dataset using convolutional neural networks. Sci. Rep. 2021, 11, 863. [CrossRef] [PubMed]
- 26. Cai, W.; Hu, D. QRS complex detection using novel deep learning neural networks. IEEE Access 2020, 8, 97082–97089. [CrossRef]
- Sodmann, P.; Vollmer, M.; Nath, N.; Kaderali, L. A convolutional neural network for ECG annotation as the basis for classification of cardiac rhythms. *Physiol. Meas.* 2018, 39, 104005. [CrossRef] [PubMed]

Short Single-Lead ECG Signal Delineation-Based Deep Learning Implementation in Automatic Atrial Fibrillation Identification

ORIGINA	ALITY REPORT			
SIMILA		2% RNET SOURCES	14% PUBLICATIONS	7% STUDENT PAPERS
PRIMAR	Y SOURCES			
1	Submitted to Student Paper	Sriwijaya	University	1 %
2	"Identification Biomarkers a Hypertrophic	n of Poten Ind Biologi Cardiomy	ang, Zhaoxia F tial Diagnostic cal Pathways opathy Based '', Genes, 2022	in on
3	assets.resear	chsquare.	com	1 %
4	www.arxiv-va	inity.com		1 %
5	Darmawahyu Computer-Aid Application to	n, Ade Iriar Ini et al. "D ded Fetal E D Heart Sta n for Cong	ni Sapitri, Anni Deep Learning Echocardiogra Andard View Enital Heart D	-Based phy:

Electrocardiogram", Springer Science and

Business Media LLC, 1980 Publication

14	hadaeeq.com Internet Source	<1%
15	github.com Internet Source	<1%
16	Submitted to National Institute of Technology, Hamirpur Student Paper	<1%
17	Jilong Wang, Renfa Li, Rui Li, Bin Fu. "A knowledge-based deep learning method for ECG signal delineation", Future Generation Computer Systems, 2020	<1%
18	doctorpenguin.com Internet Source	<1%
10		
19	Submitted to Arabian Gulf University Student Paper	<1%
20		<1 % <1 %

transforms", Indonesian Journal of Electrical Engineering and Computer Science, 2021

Publication

22	Hyeonjeong Lee, Miyoung Shin. "Learning Explainable Time-Morphology Patterns for Automatic Arrhythmia Classification from Short Single-Lead ECGs", Sensors, 2021 Publication	<1%
23	Submitted to Università di Bologna Student Paper	<1%
24	WWW.MDPI.COM Internet Source	<1%
25	www.coursehero.com Internet Source	<1%
26	Bittu Kumar. "Comparative Performance Evaluation of Greedy Algorithms for Speech Enhancement System", Fluctuation and Noise Letters, 2020 Publication	<1%
27	Submitted to University College London Student Paper	<1%
28	Allen Jong-Woei Whang, Yi-Yung Chen, Wei- Chieh Tseng, Chih-Hsien Tsai, Yi-Ping Chao, Chieh-Hung Yen, Chun-Hsiu Liu, Xin Zhang. "Pupil Size Prediction Techniques Based on Convolution Neural Network", Sensors, 2021 Publication	<1%

29	Siti Nurmaini, Alexander Edo Tondas, Annisa Darmawahyuni, Muhammad Naufal Rachmatullah et al. "Robust detection of atrial fibrillation from short-term electrocardiogram using convolutional neural networks", Future Generation Computer Systems, 2020 Publication	<1%
30	Michael T. Ohradzansky, J. Sean Humbert. "Lidar-Based Navigation of Subterranean Environments Using Bio-Inspired Wide-Field Integration of Nearness", Sensors, 2022 Publication	<1%
31	Submitted to University of Computer Studies Student Paper	<1%
32	Menaa Nawaz, Jameel Ahmed. "Anomaly Detection and Classification of Physiological Signals in IoT- Based Healthcare Framework", Research Square Platform LLC, 2021 Publication	<1%
33	"Information and Communication Technology and Applications", Springer Science and Business Media LLC, 2021 Publication	<1%
34	cora.ucc.ie Internet Source	<1%
35	Manoj Kumar Ojha, Sulochna Wadhwani, Arun Kumar Wadhwani, Anupam Shukla.	<1%

"Automatic detection of arrhythmias from an
ECG signal using an auto-encoder and SVM
classifier", Physical and Engineering Sciences
in Medicine, 2022

Publication

36	Yu Li. "Design of ECG Signal Detection Circuit Based on Pacing Pulse Suppression", 2021 IEEE International Conference on Electronic Technology, Communication and Information (ICETCI), 2021 Publication	<1%
37	M. R. Homaeinezhad, A. Ghaffari, H. Najjaran Toosi, M. Tahmasebi, M. M. Daevaeiha. "Optimal Delineation of Ambulatory Holter ECG Events via False-Alarm Bounded Segmentation of a Wavelet-Based Principal Components Analyzed Decision Statistic", Cardiovascular Engineering, 2010 Publication	<1%
38	deepai.org Internet Source	<1%
39	www.nepjol.info Internet Source	<1%

40 www.netonnet.no
Internet Source

<1%

Gamal G. N. Geweid, Mahmoud A. Abdallah.

"A New Automatic Identification Method of

<1%

Heart Failure Using Improved Support Vector Machine Based on Duality Optimization Technique", IEEE Access, 2019

Publication

42	dspace.vsb.cz Internet Source	<1%
43	iitis.pl Internet Source	<1%
44	iopscience.iop.org Internet Source	<1%
45	www.frontiersin.org Internet Source	<1%
46	Ozal Yildirim, Muhammed Talo, Edward J. Ciaccio, Ru San Tan, U Rajendra Acharya. "Accurate deep neural network model to detect cardiac arrhythmia on more than 10,000 individual subject ECG records", Computer Methods and Programs in Biomedicine, 2020 Publication	<1%
47	Ria Nova, Siti Nurmaini, Radiyati Umi Partan, Sukman Tulus Putra. "Automated image segmentation for cardiac septal defects based on contour region with convolutional neural networks: A preliminary study", Informatics in Medicine Unlocked, 2021 Publication	<1%

48	Saman Parvaneh, Jonathan Rubin, Asif Rahman, Bryan Conroy, Saeed Babaeizadeh. "Analyzing single-lead short ECG recordings using dense convolutional neural networks and feature-based post processing to detect atrial fibrillation", Physiological Measurement, 2018 Publication	<1%
49	Yong-Yeon Jo, Joon-myoung Kwon, Ki-Hyun Jeon, Yong-Hyeon Cho et al. "Detection and classification of arrhythmia using an explainable deep learning model", Journal of Electrocardiology, 2021 Publication	<1%
50	d-nb.info Internet Source	<1%
51	www.researchgate.net Internet Source	<1%
52	Berrin Küçüktürkmen, Wali Inam, Fadak Howaili, Mariam Gouda, Neeraj Prabhakar, Hongbo Zhang, Jessica M. Rosenholm. "Microfluidic-Assisted Fabrication of Dual- Coated pH-Sensitive Mesoporous Silica Nanoparticles for Protein Delivery", Biosensors, 2022 Publication	<1%

53

Hans Friedrich Stabenau, Christopher P. Bridge, Jonathan W. Waks. "ECGAug: A novel method of generating augmented annotated electrocardiogram QRST complexes and rhythm strips", Computers in Biology and Medicine, 2021

<1%

Publication

54

Siti Nurmaini, Radiyati Umi Partan, Wahyu Caesarendra, Tresna Dewi et al. "An Automated ECG Beat Classification System Using Deep Neural Networks with an Unsupervised Feature Extraction Technique", Applied Sciences, 2019

<1%

Publication

Exclude quotes

Off

Exclude matches

Off

Exclude bibliography O